



Larson Systems Inc.

13847 Aberdeen Street NE
Ham Lake, MN 55304-6789
www.larsonsystems.com

Phone: 763-780-2131
Fax: 763-780-2182
Email: info@larsonsystems.com

Packing Instructions for Manual Testers


(SDHT, DHT, CDHT, ECT, VST, SHC, FDHT)

The best way to ship your tester is in the original reusable box and packing material that it came in. When packing the tester, please send all parts and accessories with the tester, including the power supply and the handle. For best results, follow the steps below.


1. Remove the handle, handle lock knob, power supply and wrap separately in bubble wrap or packing paper.



2. Adjust the upper assembly so the distance between the blue castings is 5.25 inches and make sure the upper and lower platforms are not touching one another. Tighten the three Quick Release Handles / clamps on the upper assembly so it does not move up and down the support rods.

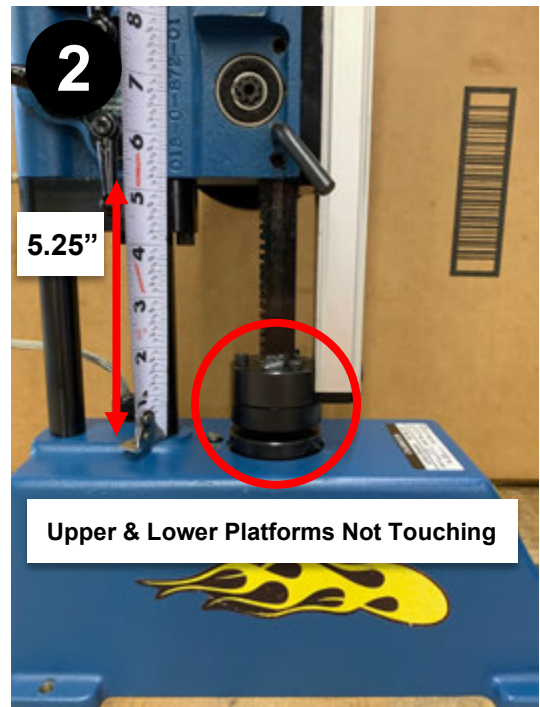

3. Engage the micro length adjust (if you have one) and tighten the gear rack lock knob. If you have quick release handles, face them forward.

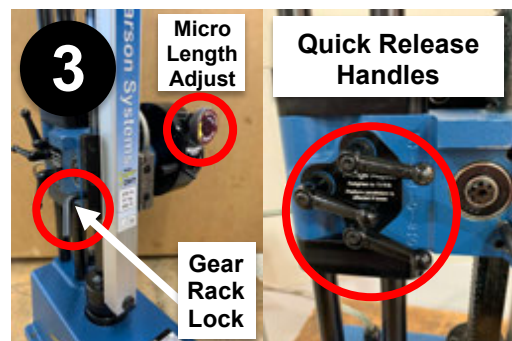

4. Enclose the tester in a plastic bag.



5. Place the tester in the foam insert, making sure it is aligned and fits snugly.



6. Slide the foam insert into the cardboard box.
7. Place the wrapped handle, handle lock knob and power supply in the side opening of the foam insert, so that they do not knock against the tester during transit. Add packing material as needed to immobilize.



8. Include paperwork (quote, purchase order, or service note) with the tester.

On your paperwork, **please record your 6-digit UPS account number.**

9. Seal box and address to:

Larson Systems Inc.

ATTN: Service

13847 Aberdeen Street NE

Ham Lake, MN 55304

NOTE:

If you do not have the original shipping box or packing materials, use a double walled box that allows for at least 2" of packing space on all 6 sides of the tester. Use packing material to keep the tester and parts immobile.